



This is a peer-reviewed, post-print (final draft post-refereeing) version of the following published document and is licensed under Creative Commons: Attribution-Noncommercial-No Derivative Works 4.0 license:

**Tiller, Nicholas B., Turner, Louise A ORCID logoORCID:  
<https://orcid.org/0000-0002-0153-7075>, Hart, John and  
Casaburi, Richard (2021) Airflow dynamics and exhaled-breath  
temperature following cold-water ingestion. *Respiratory  
Physiology and Neurobiology*, 284. Art 103564.  
[doi:10.1016/j.resp.2020.103564](https://doi.org/10.1016/j.resp.2020.103564)**

Official URL: <https://doi.org/10.1016/j.resp.2020.103564>

DOI: <http://dx.doi.org/10.1016/j.resp.2020.103564>

EPrint URI: <https://eprints.glos.ac.uk/id/eprint/8952>

#### **Disclaimer**

The University of Gloucestershire has obtained warranties from all depositors as to their title in the material deposited and as to their right to deposit such material.

The University of Gloucestershire makes no representation or warranties of commercial utility, title, or fitness for a particular purpose or any other warranty, express or implied in respect of any material deposited.

The University of Gloucestershire makes no representation that the use of the materials will not infringe any patent, copyright, trademark or other property or proprietary rights.

The University of Gloucestershire accepts no liability for any infringement of intellectual property rights in any material deposited but will remove such material from public view pending investigation in the event of an allegation of any such infringement.

PLEASE SCROLL DOWN FOR TEXT.

# AIRFLOW DYNAMICS AND EXHALED-BREATH TEMPERATURE FOLLOWING COLD-WATER INGESTION

Nicholas B. Tiller a,\* , Louise A. Turner b, John Hart c, Richard Casaburi a

**a** Institute of Respiratory Medicine and Exercise Physiology, The Lundquist Institute for Biomedical Innovation at Harbor-UCLA Medical Center, Torrance, CA, United States

**b** School of Sport and Exercise, University of Gloucestershire, Gloucester, UK

**c** Centre for Sports Engineering Research, Sheffield Hallam University, Sheffield, UK

## ABSTRACT

*Introduction:* Drinking cold water evokes decreases in spirometric indices of lung function. We studied whether this could be explained by changes in exhaled-breath temperature (EBT), airflow dynamics, and spirometer measurement sensitivity.

*Methods:* In a randomized/crossover design, 10 healthy adults consumed 1000 mL refrigerated water ( $2.1 \pm 0.64$  °C) or water at room temperature ( $19.4 \pm 0.5$  °C), with EBT assessed at baseline and at 5, 10, 15 and 30-min post-ingestion. The influence of EBT on pneumotachograph measurement characteristics was modelled using computational fluid dynamics (CFD).

*Results:* At 5-min post-ingestion, EBT was lower ( $p < 0.001$ ) following the ingestion of cold water versus water at room-temperature ( $31.7 \pm 1.1$  vs.  $33.0 \pm 0.9$  °C), and remained lower until 30-min post-ingestion. At a flow of  $8 \text{ L s}^{-1}$ , a decrease in EBT of  $2.1$  °C (as observed following cold-water ingestion) was modelled to underpredict lung volume by 0.7%.

*Conclusions:* Cold water reduces EBT below baseline but effects pneumotachograph measurements only negligibly. Therefore, decreased lung function following cold-water ingestion likely has a physiological explanation which warrants further study.

**Keywords:** Airflow; Lung function; Spirometry

---

\* Corresponding author at: The Lundquist Institute, 1124 West Carson St., CDCRC Building, Torrance, CA 90502, United States. E-mail address: nicholas.tiller@lundquist.org (N.B. Tiller).

# 1. INTRODUCTION

Spirometry is a common pulmonary function test (PFT) used in the diagnosis and monitoring of respiratory disorders (Miller et al., 2005; Graham et al., 2019). In addition to providing standardized criteria for maneuver quality, the ATS/ERS suggest that optimal and repeatable results are more likely if a patient abstains from vigorous exercise for 1 h, smoking or vaping for 1 h, large meals for 2 h, and alcohol for 4 h before a given test. There are no clear guidelines pertaining to fluid ingestion as it relates to spirometry, aside from the recommendation that “drinking water should be available” (Graham et al., 2019).

Two recent studies from our group suggest that water, ingested up to 30 min before spirometry, may negatively impact on lung function. In the first of these studies, 500–700 mL tap-water evoked significant decreases in forced vital capacity (FVC,  $-2.3\%$ ) and forced expiratory volume in 1 s ( $FEV_1$ ,  $-2.9\%$ ) in healthy subjects (Turner et al., 2015). We observed no such changes with a volume-matched food bolus, indicating that the decreases in lung function following fluid ingestion were independent of gastric load, per se. In the second study, we showed that 1000 mL of refrigerated water ( $\sim 3^\circ\text{C}$ ) significantly reduced FVC,  $FEV_1$ ,  $FEV_1/FVC$ , and forced expiratory flow measured between 25 and 75% of the exhalation ( $FEF_{25-75}$ ) in the range of 5 - 10%. Furthermore, the decreases were significantly greater than those observed with an equivalent volume of water at room-temperature (Turner et al., 2016). We thereby concluded that ingesting a large bolus of water had the potential to reduce lung function via a mechanism that was likely temperature-dependent.

We can conceive two potential physiological explanations for these findings. First, the autonomic nervous system plays an important role in regulating airway function (van der Velden and Hulsmann, 1999). Ingesting cold water has been shown to increase vagal tone (Chiang et al., 2010), which might trigger airway mucous production and bronchoconstriction in susceptible groups (Undem and Kollarik, 2005). Second, cold air can evoke a pro-inflammatory hyper-responsiveness in the airway (Cockcroft and Davis, 2006), and it is plausible that the ingestion of cold water may exert a similar effect due to the trachea’s close anatomical proximity to the upper-GI tract (laryngopharynx and oesophagus). Both of these hypotheses are yet to be tested.

A third possible explanation for a decrease in spirometric values following cold-water ingestion is a decrease in exhaled-breath temperature (EBT) (via indirect cooling of the upper-airway), and the consequent effect of gas temperature on spirometer measurement (Miller and Sigsgaard, 1994). The pneumotachograph is the most widely-used device in laboratory-based lung function testing (de Jongh, 2008). During an expiratory maneuver, a transducer measures pressure differentials ( $\Delta P$ )

across a capillary tube bank. On the basis that pressure and laminar flow are proportional (Button, 2015), an analogue  $\Delta P$  signal is used to calculate flow, which is integrated to volume. The  $\Delta P$  is dependent on gas viscosity which increases with temperature (Miller et al., 2005). As a result, a potential source of error is that a change in the temperature of expired gas (from ingesting cold fluids) may alter airflow dynamics, and disrupt the flow-pressure relationship on which the pneumotachograph output is based.

There is also a large discrepancy between the ambient temperature (that at which the pneumotachograph is calibrated) and that of the exhaled gas; this, in turn, would be expected to influence the calculated flows and volumes. Accordingly, a BTPS correction factor (which assumes that gas temperature in the measuring device is equivalent to body temperature; i.e., 37 °C) is applied to the outcome variables. A second potential source of error, therefore, is a cold-water-induced decrease in the exhaled gas temperature below the anticipated 37 °C, thereby invalidating one of the assumptions of the BTPS equation.

To further elucidate the mechanical factors by which cold-water ingestion might influence spirometry, several questions need to be addressed. First, is whether ingesting cold water reduces exhaled-breath temperature (EBT) in healthy subjects. Second, is whether the reduction in EBT induced by cold water ingestion is sufficient to influence airflow dynamics and, therefore, the measurement characteristics of a commercially-available pneumotachograph. Data to this effect would edify standardization guidelines for PFTs, and inform further mechanistic studies into the nature of lung function decline following cold-water ingestion. Given that EBT is widely utilized as a means of monitoring day-to-day perturbations in airway inflammation (Popov et al., 2017), data on cold-water ingestion as a potential confounding factor in the assessment of EBT may also prove insightful. Accordingly, the aims of this randomized, cross-over trial were to evaluate the effects of fluid ingestion on EBT in healthy adults, and to use computational fluid dynamics (CFD) to model the effect of perturbations in gas temperature (and pressure) on pneumotachograph measurements.

## 2. METHODS

### 2.1. SUBJECTS

Ten healthy, recreationally-active adults (5 male/5 female) volunteered to participate (age =  $36 \pm 7$  y; mass =  $87.4 \pm 31.8$  kg; stature =  $1.74 \pm 0.80$  m). After providing written, informed consent, subjects were instructed to attend the laboratory following an overnight fast, and to abstain from taking any

fluid the morning of their visits. The study was approved by the institution's Research Ethics Committee, and performed in accordance with the 1964 Declaration of Helsinki.

## 2.2. EXPERIMENTAL OVERVIEW

Subjects attended the laboratory on three occasions separated by at least 24 h. At the first visit, they performed basic anthropometry, baseline spirometry, and were accustomed to measures of exhaled-breath temperature (EBT). At the second and third visits, subjects performed baseline tests of EBT, after which they consumed a single bolus of cold- or room-temperature water with follow-up tests of EBT performed periodically for 30 min. The order of trials was randomized and counterbalanced, and performed at the same time of day to eliminate the influence of circadian variance. The effect of exhaled gas temperature on measurement characteristics of the pneumotachograph was modelled using CFD (see below).

## 2.3. SPIROMETRY

Baseline pulmonary volumes, capacities, and flows were assessed via spirometry. Subjects performed between three and eight FVC maneuvers into a two-way disposable mouthpiece connected to a portable pneumotachograph (Alpha Touch; Vitalograph Ltd., Buckingham, England). Subjects were seated, had the nose occluded, and verbal encouragement was given to ensure consistent efforts. Spirometry was performed in accordance with ATS/ERS guidelines (Miller et al., 2005), and all values were expressed in absolute terms and as percentages of predicted norms (Quanjer et al., 2012).

## 2.4. EXHALED-BREATH TEMPERATURE


Exhaled-breath temperature was assessed during tidal breathing using a hand-held thermometer (X-Halo; Delmedica Investments, Singapore) using protocols previously described (Popov et al., 2007). Briefly, participants were required to inhale through the nose and exhale through the mouth into a one-way antimicrobial filter. The EBT device comprised a metal core containing a high-precision thermal sensor housed within a 300 mL thermo-insulated chamber. Participants were asked to maintain normal tidal breathing until the metal core reached a thermal balance in the mixing chamber (3–6 min), at which point peak-EBT was recorded. Following two baseline measures spaced 10 min apart to deduce reproducibility, participants were given 10 min to consume 1000 mL of refrigerated water ( $2.1 \pm 0.6$  °C) or water at room temperature ( $19.4 \pm 0.5$  °C). Exhaled-breath temperature measures were repeated at 5, 10, 15, and 30 min post-ingestion.

## 2.5. WITHIN- AND BETWEEN-DAY REPRODUCIBILITY OF MEASURES

Within-day reproducibility of EBT was determined by comparing two sets of baseline measures recorded before and after 10 min passive rest. Between-day reproducibility was determined by re-assessing baseline values at the second visit > 24 h later. There were no systematic differences in measurements ( $p > 0.05$ ), and the between-occasion reliability was excellent ( $CV = 0.66\%$ ;  $SEM = 0.09$  °C;  $ICC = 0.84$ ). Using similar procedures and identical apparatus to the present study, we recently published strong within- and between-day reproducibility of our spirometric assessments (all  $CV < 5\%$ ; all  $SEM < 5\%$ ; all  $ICC > 0.94$ ) (Tiller et al., 2019).

## 2.6. COMPUTATIONAL FLUID DYNAMICS

Computational fluid dynamics was used to model the influence of exhaled-breath temperature on spirometer measurements. The numerical calculation of flow was accomplished through solution of continuity, Navier–Stokes, energy and turbulence model equations (Versteeg and Malalasekera, 1995). Calculations were performed using commercially-available software (Fluent version 17.1.0; ANSYS, Pennsylvania, U.S.A.). A geometric representation of the pneumotachograph and associated equipment, suitable for simulation, was first created with a 22.5° rotational periodic geometric assumption using computer-aided design (Fig. 1). This was subsequently discretized into 15.3 million polyhedral elements, and the geometry represented with finite volumes in which flow calculations were iteratively performed.

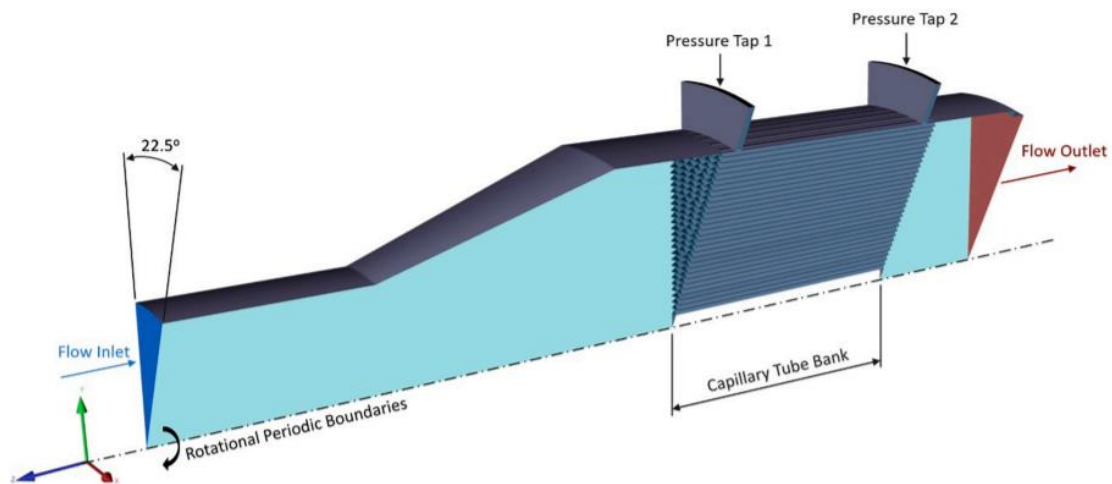

**FIGURE 1 MODELLED PNEUMOTACH GEOMETRY WITH A ROTATIONAL PERIODICITY OF 22.5°. THE GEOMETRY OF THE PNEUMOTACH CAN BE APPROXIMATED AS AXIALLY REPEATING, ALLOWING THE USE OF ROTATIONAL PERIODIC BOUNDARY ASSUMPTIONS THAT REDUCE OVERALL COMPUTATIONAL EXPENSE OF THE SIMULATION.**

With the body temperature of the pneumotachograph held at a constant 20 °C (i.e., that at which it was calibrated), the effect of various gas temperatures (20, 22, 24, 26, 28, 30, 32, 34 °C) on the

measured pressure drop ( $\Delta P$ ) across the capillary tube bank was simulated at fixed physiological flow rates of 1, 4, 8, 12, and 16 L s<sup>-1</sup>. Physical gas properties were specified using temperature-dependent polynomials. A pneumotachograph operates on the principle that pressure drop and laminar flow through the body are proportional. For a known  $\Delta P$  signal, it is possible to calculate flow rate as a factor of time, and thereby interpolate volume. However, because  $\Delta P$  is affected by temperature of the gas passing through the device, a discordance between the calibration gas temperature and the exhaled gas temperature will introduce discrepancies in the calculated flow (that is, unless a temperature correction has been applied). Through the simulation process (based on a representative flow-volume curve in a healthy subject with normal lung function), a series of  $\Delta P$ -flow curves were obtained for each gas temperature. From these curves, it was possible to calculate the discrepancy in reported flow and volume that would result from a pneumotachograph calibrated at room temperature (20 °C). Accordingly, we determined the effect of changes in gas temperature alone, as evoked by cold-water ingestion, on predicted pneumotachograph flow/volume metrics.

## 2.7. DATA ANALYSIS

Descriptive and inferential statistics were calculated using SPSS 24 for Windows (IBM; Illinois, U.S.A.). Reproducibility was assessed using coefficient of variation (CV), standard error of measurement (SEM), and intra-class correlation coefficients (ICC). Exhaled breath temperature following the ingestion of cold- and room-temperature water was compared using a two-factor (condition  $\times$  time) Repeated-Measures ANOVA, with a critical alpha level of 0.05. The assumption of equal variance was assessed via Mauchly's Test of Sphericity and, if violated ( $p < 0.05$ ), a Greenhouse-Geisser correction was applied. On significant interactions, follow-up pairwise comparisons were performed using a Bonferroni-adjusted alpha level of 0.01. Effect size (Cohen's  $d$ ) was used to quantify the magnitude of the difference between group means (0.2 = small; 0.5 = medium; 0.8 = large effect) (Cohen, 1977). Data were presented as mean  $\pm$  standard deviation (SD).

## 3. RESULTS

### 3.1. SPIROMETRY

Lung function was within normal limits: FVC = 103  $\pm$  18% Pred; FEV1 = 87  $\pm$  18% Pred; FEV1/VC = 85  $\pm$  8%; peak expiratory flow = 106  $\pm$  22% Pred.

### 3.2. EXHALED BREATH TEMPERATURE

Exhaled-breath temperature at baseline and in response to the ingestion of cold- and room-temperature water is shown in Table 1. Baseline EBT was not different between the two experimental visits ( $p = 0.269$ ,  $d = 0.25$ ). Mean drink temperature was  $2.1 \pm 0.6$  °C in the cold-water condition (range 1–3 °C) and  $19.4 \pm 1.5$  °C in the room-temperature condition (range 17–21.5 °C). Relative to baseline, EBT at 5 min post-ingestion had decreased significantly with both cold water ( $p < 0.001$ ,  $d = 2.57$ ) and room-temperature water ( $p = 0.005$ ,  $d = 0.94$ ), and in both cases remained below baseline until the final measurement at 30 min ( $p < 0.01$ ). When comparing between the conditions, there were main-effects showing a lower EBT with cold water ( $F[1,9] = 62.90$ ,  $p < 0.001$ ), and a condition  $\times$  time interaction ( $F[2,21,36] = 10.72$ ,  $p = 0.001$ ). Pairwise comparisons revealed that EBT was significantly lower following the ingestion of cold water relative to room-temperature water at 5, 10, and 15 min ( $p < 0.001$ ; Table 1). Differences at 30 min were worthy of note, but did not reach statistical significance ( $p = 0.059$ ).

**TABLE 1 EXHALED-BREATH TEMPERATURE AT BASELINE AND FOLLOWING THE INGESTION OF COLD- OR ROOM-TEMPERATURE WATER.**

	<b>Cold (2.1°C)</b>	<b>Room (19.4°C)</b>	<b>*p</b>	<b>d</b>
<b>Baseline</b>	33.8 $\pm$ 0.4	33.7 $\pm$ 0.5	0.269	0.25
<b>+5 min</b>	31.7 $\pm$ 1.1*	33.0 $\pm$ 0.9*†	<0.001	1.34
<b>+10 min</b>	32.6 $\pm$ 0.6*	33.2 $\pm$ 0.6*†	<0.001	1.06
<b>+15 min</b>	32.5 $\pm$ 0.6*	33.3 $\pm$ 0.5*†	<0.001	1.46
<b>+30 min</b>	32.8 $\pm$ 0.5*	33.3 $\pm$ 0.8*	0.059	0.74

Mean  $\pm$  SD,  $n = 10$ .  $d =$  Cohen's  $d$  effect size (0.2 = small, 0.5 = medium, 0.8 = large effect) (17). \*significantly different versus respective baseline; †significantly different versus cold water.

### 3.3. COMPUTATIONAL FLUID DYNAMICS


The influence of gas temperature on pressure differentials across the tube bank is shown in Table 2. The magnitude of the pressure drop increased congruent with flow rate and, at each of the five flow rates (1, 4, 8, 12, and 16 L s<sup>-1</sup>),  $\Delta P$  was lower at higher gas temperatures. From these data, we were able to model the influence of EBT perturbations on  $\Delta P$  and the subsequent expiratory flow-volume curve. In a pressure transducer calibrated with an ambient gas of 20 °C, an EBT of 33.8 °C (baseline) and 31.7 °C (post- cold-water ingestion) would result in the underprediction of volume by 5.2 and 4.5%, respectively (Fig. 2). At an example flow rate of 8 L s<sup>-1</sup>, a decrease in gas temperature from 33.8–31.7 °C attenuated  $\Delta P$  by 3.2 Pa (0.8%). Thus, in this scenario, a cold-water-induced decrease in EBT of 2.1 °C results in a difference between predicted volumes of 0.7%.



**TABLE 2 THE MODELLED INFLUENCE OF GAS TEMPERATURE ON PRESSURE CHANGES ACROSS THE PNEUMOTACHOGRAPH TUBE BANK.**

Flow (L s <sup>-1</sup> )	Pressure difference across pneumotachograph (Pa)		
	20°C	28.5°C (% Diff.)	34.5°C (% Diff.)
1	-43.9	-42.6 (3.1)	-41.7 (5.3)
4	-197.9	-191.7 (3.2)	-187.6 (5.5)
8	-426.5	-413.1 (3.2)	-404.1 (5.5)
12	-664.2	-643.5 (3.2)	-629.5 (5.5)
16	-907.4	-877.0 (3.5)	-858.0 (5.8)

% Diff. is relative to pressure at 20 °C

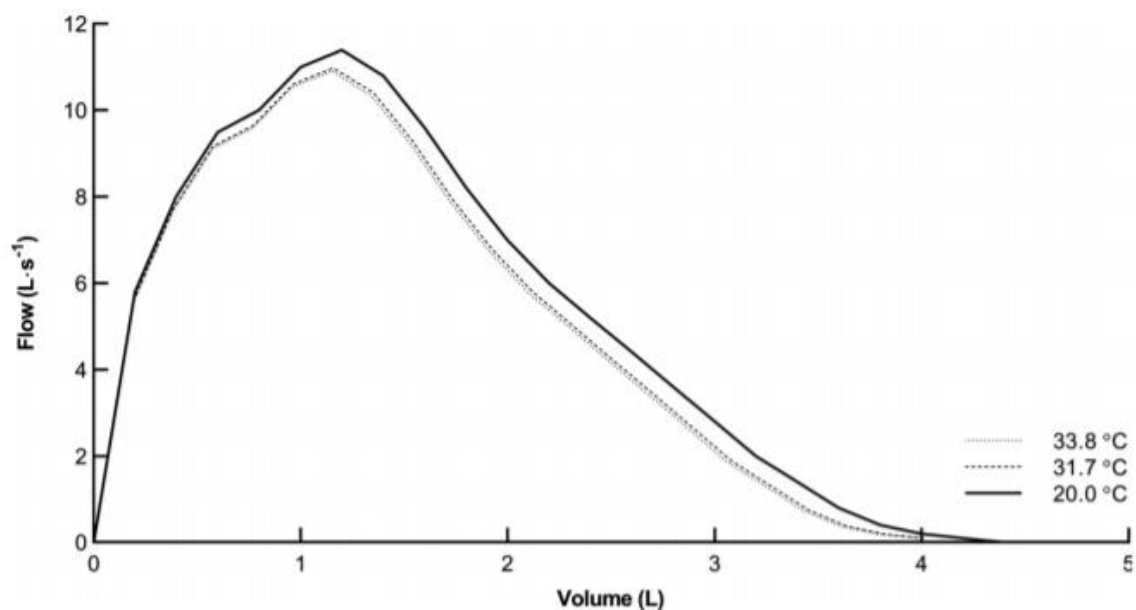

**FIGURE 2 MODELLED INFLUENCE OF GAS TEMPERATURE ON A TYPICAL EXPIRATORY FLOW-VOLUME CURVE. IN A PRESSURE TRANSDUCER CALIBRATED WITH A GAS OF 20 °C (STANDARD ROOM TEMPERATURE), AN EBT OF 33.8 °C (BASELINE) AND 31.7 °C (POST- COLD-WATER INGESTION) RESULT IN AN UNDERESTIMATION OF THE CALCULATED VOLUME BY 5.2 AND 4.5%, RESPECTIVELY. THE EBT DECREASE FOLLOWING COLD-WATER INGESTION (2.1 °C) RESULTS IN A 0.7% UNDERPREDICTION OF VOLUME.**

## 4. DISCUSSION

The aims of this study were to evaluate the effects of fluid ingestion on EBT in healthy adults, and to use computational fluid dynamics to model the effect of perturbations in gas temperature (and pressure) on pneumotachograph measurement sensitivity. We made several observations: i) the ingestion of both cold water and room-temperature water resulted in significant decreases in EBT, with values remaining below baseline for at least 30 min; ii) cold-water ingestion decreased EBT to a

significantly greater magnitude than water at room temperature; and iii) the decrease in EBT following cold-water ingestion was calculated to influence the pneumotachograph flow-volume measurement by < 1%. These data have implications for the clinical assessment of both spirometry and EBT.

#### 4.1. TECHNICAL CONSIDERATIONS

There are several considerations that should predicate the interpretation of our data. First, as discussed below, certain factors might confound the measurement of EBT, including food, exercise, cigarette-smoking, and circadian variance (Carpagnano et al., 2016, 2017; Kralimarkova et al., 2012, 2014; Svensson et al., 2012). To mitigate these factors, we recruited non-smokers, instructed our subjects to attend the laboratory having abstained from food, fluid, and exercise on the morning of the test, and we assessed EBT at the same time of day in both experimental trials (i.e., 08:00–09:00). We also demonstrate excellent within- and between-day reproducibility of our EBT measures: no systematic differences in measurements ( $p > 0.05$ ); CV = 0.66%; SEM = 0.09 °C; ICC = 0.84. As such, we are confident that our data reflect the true EBT responses to cold-water ingestion.

Second, our model of EBT and airflow dynamics is only relevant when assessing lung function via the Fleisch or Lilly pneumotachograph (i.e., those deriving flow via pressure differentials across a screen or capillary tube bank). Other frequently-used devices include wet/dry volume-measurement spirometers, and flow measurement devices operating under different principles (e.g., mass flow meters), and there are systematic differences in the data obtained among the various spirometers (Brouwer et al., 2007; Gerbase et al., 2013; Swart et al., 2003). As such, although pneumotachographs are generally considered to be the best (Miller et al., 1997) and most widely-used (de Jongh, 2008) means of measuring forced expiratory maneuvers, further studies are needed to assess the effects of cold-water-induced changes in airflow dynamics with other devices.

Finally, it is worth noting that our airflow model is based on the standard, non-heated pneumotachograph that is in widespread clinical use (Miller and Sigsgaard, 1994). Some devices contain a heated element that conditions the expired air in order to reduce surface condensation in the tube bank that may occur during repeated expiratory maneuvers, but this is unlikely to reduce measurement inaccuracies that result from changes in gas temperature.

## 4.2. EXHALED-BREATH TEMPERATURE AND COMPUTATIONAL FLUID DYNAMICS

The bronchial microvasculature plays an important role in the response to airway disease (Paredi and Barnes, 2009), and the assessment of EBT has become commonplace in monitoring day-to-day perturbations in airway blood flow resulting from inflammation and exacerbation (Popov et al., 2012). Indeed, acute exacerbations in asthmatic patients (resulting from hyperreactivity and vascularization of the bronchial smooth muscle) transiently increase EBT; by contrast, chronic airway damage and reduced vascularization which characterize COPD results in lower baseline EBT values (Popov et al., 2012).

Several factors are thought to confound the measurement of EBT. Circadian variance was shown to result in EBT fluctuations of  $\sim 1.33$  °C (Carpagnano et al., 2017), while smoking a cigarette and eating snack foods have been shown to influence baseline measurements by  $\sim 0.19$  °C (Kralimarkova et al., 2014) and  $\sim 0.48$  °C (Kralimarkova et al., 2012), respectively. Following exercise, asthmatics and healthy controls exhibited increases in EBT of  $< 1.0$  °C, with no significant difference between groups (Svensson et al. 2012). To our knowledge, ours is the first study to evaluate the effect of fluid ingestion on EBT measurement. The data show that a bolus of refrigerated water decreased EBT to a far greater magnitude ( $- 2.1$  °C) than that observed from other confounders. Moreover, the decrease had only partially recovered (to  $- 1.0$  °C) at 30 min post-ingestion (Table 1). Accordingly, patients using EBT as a means of monitoring airway inflammation should abstain from drinking large volumes of fluid, particularly cold fluid, for at least 30–60 min before a given assessment.

To evaluate the effect of cold-water ingestion on spirometer measurement, we first modelled the broad effects of gas temperature on airflow dynamics in a standard, non-heated pneumotachograph. The model assumed that the device was calibrated using an ambient gas at 20 °C. At an expiratory flow of  $8.0 \text{ L s}^{-1}$ , we calculated that an exhaled gas temperature of 33.8 °C (baseline EBT) would result in a  $\Delta P$  across the tube bank that is 22.4 Pa (5.5%) larger than that elicited by an ambient temperature exhalate. The result would be a flow underprediction of 5.2% (Table 2). To accommodate this considerable error, a BTPS correction factor is applied which assumes that gas temperature in the measuring device is equivalent to body temperature (i.e., 37 °C). However, there are numerous studies showing baseline EBT to be below 37 °C in various subgroups, including healthy controls (33.2–34.8 °C, Popov et al., 2007; García et al., 2013; Svensson et al., 2012), asthmatics (33.7–35.5 °C, Popov et al., 2007; Svensson et al., 2012, 2014; García et al., 2013), and patients with COPD (34.0–34.6 °C, Lázár et al., 2014). We presently report a baseline EBT in our healthy cohort of  $\sim 33.8 \pm 0.4$  °C, which mirrors data from Svensson et al. (2012), and corroborates the general consensus. As such, to mitigate unnecessary errors in spirometric measurement, we concur with others who suggest that the BTPS

correction factor for expiratory gas should be adapted to the actual gas conditions in the pneumotachograph (Normand et al., 2007).

We next assessed the effects of a change in EBT on spirometer airflow dynamics. We showed that a cold-water-induced decrease in EBT of 2.1 °C would alter the linear flow-pressure relationship, and decrease the volume output by 0.7%. Our earlier studies show a decrease in FVC, FEV<sub>1</sub>, and MEF<sub>25-75</sub> in the region of 5–10% following cold-water ingestion (Turner et al., 2015, 2016). These decreases are of a far greater magnitude than can be explained by our current model of pneumotachograph airflow temperature considerations. At present we can only speculate on the physiological mechanisms that underpin lung function decline following cold-water ingestion. It was initially thought that cold-water ingestion may evoke a pro-inflammatory hyperresponsiveness in the airway, in a similar fashion to that observed with cold air (Cockcroft and Davis, 2006). However, Svensson et al. (2012) reported larger post-exercise decreases in FEV<sub>1</sub> in those individuals with higher EBT, suggesting that EBT increases under conditions of acute airway inflammation. We currently report decreases in EBT following cold-water ingestion, thereby potentially discounting airway inflammation and/or hyperresponsiveness as a causative factor. Further research into these mechanisms may have important implications for routine pulmonary function testing.

In conclusion, we observed large and sustained decreases in exhaled breath temperature following the ingestion of cold water. The magnitude of the decrease exceeds that seen with other confounding variables and, as such, abstaining from fluid ingestion for at least 30 min prior to a test should be integrated into standard EBT assessment guidelines. However, the decreases in EBT influenced spirometer measurements only negligibly (<1%), suggesting that cold-water-induced decreases in spirometric output likely have a physiological mechanism that warrants further study.

#### ***Declaration of Competing Interest***

The authors reported no declarations of interest.

#### ***Acknowledgements***

The authors would like to thank the subjects who volunteered their time to participate in this research. The corresponding author (NBT) is funded by a postdoctoral fellowship from the Tobacco-Related Disease Research Program (TRDRP; award no. T31FT1692).

## REFERENCES

- Brouwer, A.F.J., Roorda, R.J., Brand, P.L.P., 2007. Comparison between peak expiratory flow and FEV1 measurements on a home spirometer and on a pneumotachograph in children with asthma. *Pediatr. Pulmonol.* 42, 813–818. <https://doi.org/10.1002/ppul.20660>.
- Button, V.L.D.S.N., 2015. Flow transducers. *Principles of Measurement and Transduction of Biomedical Variables*. Elsevier, pp. 271–323. <https://doi.org/10.1016/B978-0-12-800774-7.00007-6>.
- Carpagnano, G.E., Ruggieri, C., Scioscia, G., Storto, M.Mlo, Zoppo, L., Foschino-Barbaro, M.P., 2016. Is the exhaled breath temperature sensitive to cigarette smoking? *COPD J. Chronic Obstr. Pulm. Dis.* 13, 642–646. <https://doi.org/10.3109/15412555.2016.1143458>.
- Carpagnano, G.E., Lacedonia, D., Malerba, M., Martinelli, D., Cotugno, G., Foschino-Barbaro, M.P., 2017. Exhaled breath temperature measurement: influence of circadian rhythm. *J. Biol. Regul. Homeost. Agents* 31, 229–235.
- Chiang, Cte, Chiu, T.W., Jong, Y.S., Chen, G.Y., Kuo, C.D., 2010. The effect of ice water ingestion on autonomic modulation in healthy subjects. *Clin. Auton. Res.* 20, 375–380. <https://doi.org/10.1007/s10286-010-0077-3>.
- Cockcroft, D.W., Davis, B.E., 2006. Mechanisms of airway hyperresponsiveness. *J. Allergy Clin. Immunol.* <https://doi.org/10.1016/j.jaci.2006.07.012>.
- Cohen, J., 1977. *Statistical Power Analysis for the Behavioral Sciences*. Routledge, New York, New York.
- de Jongh, F., 2008. Spirometers. *Breathe* 4, 251–254.
- García, G., Bergna, M., Uribe, E., Yañez, A., Soriano, J.B., 2013. Increased exhaled breath temperature in subjects with uncontrolled asthma. *Int. J. Tuberc. Lung Dis.* 17, 969–972. <https://doi.org/10.5588/ijtld.12.0657>.
- Gerbase, M.W., Dupuis-Lozeron, E., Schindler, C., Keidel, D., Bridevaux, P.O., Kriemler, S., Probst-Hensch, N.M., Rochat, T., Künzli, N., 2013. Agreement between spirometers: a challenge in the follow-up of patients and populations? *Respiration* 85, 505–514. <https://doi.org/10.1159/000346649>.
- Graham, B.L., Steenbruggen, I., Barjaktarevic, I.Z., Cooper, B.G., Hall, G.L., Hallstrand, T. S., Kaminsky, D.A., McCarthy, K., McCormack, M.C., Miller, M.R., Oropez, C.E., Rosenfeld, M., Stanojevic, S., Swanney, M.P., Thompson, B.R., 2019. Standardization of spirometry 2019 update an official American Thoracic Society and European Respiratory Society technical statement. *Am. J. Respir. Crit. Care Med.* <https://doi.org/10.1164/rccm.201908-1590ST>.

- Kralimarkova, T., Mincheva, R., Kadavil, R., John, J., Tihomirov, D., Dimitrov, V., Popov, T., 2012. Effect of energy food intake on exhaled breath temperature in healthy subjects. *Eur. Respir. J.* 40.
- Kralimarkova, T., Hristova, D., Kadavil, R., John, J., Sabu, J., Dimitrov, V., Popov, T., 2014. Short term effects of tobacco smoking on exhaled breath temperature. *Eur. Respir. J.* 44. Lázár, Z., Bikov, A., Martinovszky, F., Gálffy, G., Losonczy, G., Horváth, I., 2014. Exhaled breath temperature in patients with stable and exacerbated COPD. *J. Breath Res.* 8, 046002 <https://doi.org/10.1088/1752-7155/8/4/046002>.
- Miller, M.R., Sigsgaard, T., 1994. Prevention of thermal and condensation errors in pneumotachographic recordings of the maximal forced expiratory manoeuvre. *Eur. Respir. J.* 7, 198–201. <https://doi.org/10.1183/09031936.94.07010198>.
- Miller, M.R., Pedersen, O.F., Sigsgaard, T., 1997. Spirometry with a Fleisch pneumotachograph: upstream heat exchanger replaces heating requirement. *J. Appl. Physiol.*
- Miller, M.R., Hankinson, J., Brusasco, V., Burgos, F., Casaburi, R., Coates, A., Crapo, R., Enright, P., van der Grinten, C.P.M., Gustafsson, P., Jensen, R., Johnson, D.C., MacIntyre, N., McKay, R., Navajas, D., Pedersen, O.F., Pellegrino, R., Viegi, G., Wagner, J., 2005. Standardisation of spirometry. *Eur. Respir. J.* <https://doi.org/10.1183/09031936.05.00034805>.
- Normand, H., Normand, F., le Coutour, X., Metges, M.A., Mouadil, A., 2007. Clinical evaluation of a screen pneumotachograph as an in-line filter. *Eur. Respir. J.* 30, 358–363. <https://doi.org/10.1183/09031936.06.00148105>.
- Paredi, P., Barnes, P.J., 2009. The airway vasculature: recent advances and clinical implications. *Thorax.* <https://doi.org/10.1136/thx.2008.100032>.
- Popov, T.A., Dunev, S., Kralimarkova, T.Z., Kraeva, S., DuBuske, L.M., 2007. Evaluation of a simple, potentially individual device for exhaled breath temperature measurement. *Respir. Med.* 101, 2044–2050. <https://doi.org/10.1016/j.rmed.2007.06.005>.
- Popov, T.A., Kralimarkova, T.Z., Dimitrov, V.D., 2012. Measurement of exhaled breath temperature in science and clinical practice. *Breathe* 8, 186–192. <https://doi.org/10.1183/20734735.021811>.
- Popov, T., Kralimarkova, T., Labor, M., Plavec, D., 2017. The added value of exhaled breath temperature in respiratory medicine. *J. Breath Res.* 11. <https://doi.org/10.1088/1752-7163/AA7801>.
- Quanjer, P.H., Stanojevic, S., Cole, T.J., Baur, X., Hall, G.L., Culver, B.H., Enright, P.L., Hankinson, J.L., Ip, M.S.M., Zheng, J., Stocks, J., Schindler, C., 2012. Multi-ethnic reference values for spirometry for the 3-95-yr age range: the global lung function 2012 equations. *Eur. Respir. J.* 40, 1324–1343. <https://doi.org/10.1183/09031936.00080312>.

- Svensson, H., Nilsson, D., Bjermer, L., Tufvesson, E., 2012. Exhaled breath temperature increases after exercise in asthmatics and controls. *Respiration* 84, 283–290.  
<https://doi.org/10.1159/000335252>.
- Svensson, H., Bjermer, L., Tufvesson, E., 2014. Exhaled breath temperature in asthmatics and controls after eucapnic voluntary hyperventilation and a methacholine challenge test. *Respiration* 87, 149–157. <https://doi.org/10.1159/000355088>
- Swart, F., Schuurmans, M., Heydenreich, J., Pieper, C., Bolliger, C., 2003. Comparison of a new desktop spirometer (Spirospec) with a laboratory spirometer in a respiratory out-patient clinic. *Respir. Care* 48, 591–595.
- Tiller, N.B., Turner, L.A., Taylor, B.J., 2019. Pulmonary and respiratory muscle function in response to 10 marathons in 10 days. *Eur. J. Appl. Physiol.* 119, 509–518.  
<https://doi.org/10.1007/s00421-018-4037-2>.
- Turner, L.A., Gonzalez, J.T., Rumbold, P.L., Green, B., Brown, M., Mickleborough, T.D., Stevenson, E., 2015. The influence of drink and meal ingestion on resting pulmonary function in active individuals. *Med. Sci. Sports Exerc.* 47, 723.  
<https://doi.org/10.1249/01.mss.0000478701.16403.0d>.
- Turner, L.A., O'Hagan, C., Rumbold, P.L., 2016. Drink temperature influences resting pulmonary function in active individuals. *Med. Sci. Sports Exerc.* 48, 458–459.  
<https://doi.org/10.1249/01.mss.0000486378.67504.a3>.
- Udem, B.J., Kollarik, M., 2005. The role of vagal afferent nerves in chronic obstructive pulmonary disease. In: *Proceedings of the American Thoracic Society*. American Thoracic Society, pp. 355–360. <https://doi.org/10.1513/pats.200504-033SR>.
- van der Velden, V.H.J., Hulsmann, A.R., 1999. Autonomic innervation of human airways: structure, function, and pathophysiology in asthma. *NeuroImmunoModulation*.  
<https://doi.org/10.1159/000026376>.
- Versteeg, H.K., Malalasekera, W., 1995. *An Introduction to Computational Fluid Dynamics: The Finite Volume Method*. Pearson Education Limited.